

An anatomical illustration of a heart, showing the major blood vessels. A blue catheter is inserted into one of the vessels. Inside the catheter, a yellow, brush-like extraction device is visible, designed for lead extraction. The heart muscle is shown in a reddish-pink color, and the vessels are in shades of blue and red.

Evolve your Lead Extraction™
procedures with controlled
bidirectional rotation.

Evolution® RL
LEAD EXTRACTION™ SYSTEM



www.cookmedical.com

After receiving feedback from clinicians around the world, we've updated the Evolution RL and Evolution Shortie RL Controlled-Rotation Dilator Sheath Sets. To give you more control during the lead extraction procedure, Cook has added three new features to the already innovative line of Evolution devices: a birotational sheath; a low-profile, decagonal tip; and a responsive trigger. These three features allow you to focus on the primary task of safely removing problematic leads and also lessen the distractions that companion leads or suboptimal lead positioning can cause. The Evolution RL line of extraction sheaths combine engineering expertise with the procedural knowledge that physicians have come to expect from Cook Medical.


Birotational Sheath

- Rotate in alternating directions or continuously in either direction.
- Rotate fully or partially, depending on the length of the trigger pull.
- Resist kinking with a durable braided inner sheath.



Decagon-Shaped Tip

- Avoids tissue wrap and deflects companion leads.
- Maintains forward progression whether it rotates right or left.
- Has a low profile.

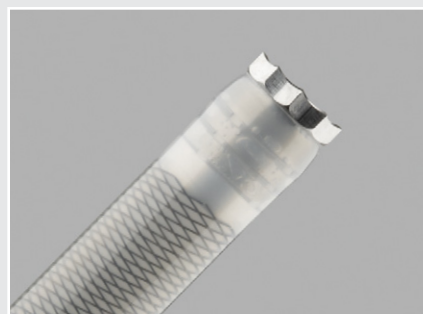

Responsive, Contoured Handle


- Centered position of the the sheath makes the device friendly to both right- and left-handed users.
- Intuitive two-stage trigger changes the direction of rotation without buttons or switches.
- Rotation indicator clearly indicates the direction of rotation.



Evolution® RL

CONTROLLED-ROTATION DILATOR SHEATH SET

The Evolution RL helps you extract leads by separating binding adhesions along the entire length of your targeted cardiac lead. The PTFE outer sheath can be used to disrupt tissue and apply countertraction. The Evolution RL comes in a range of sizes that accommodates both pacing and defibrillator leads.

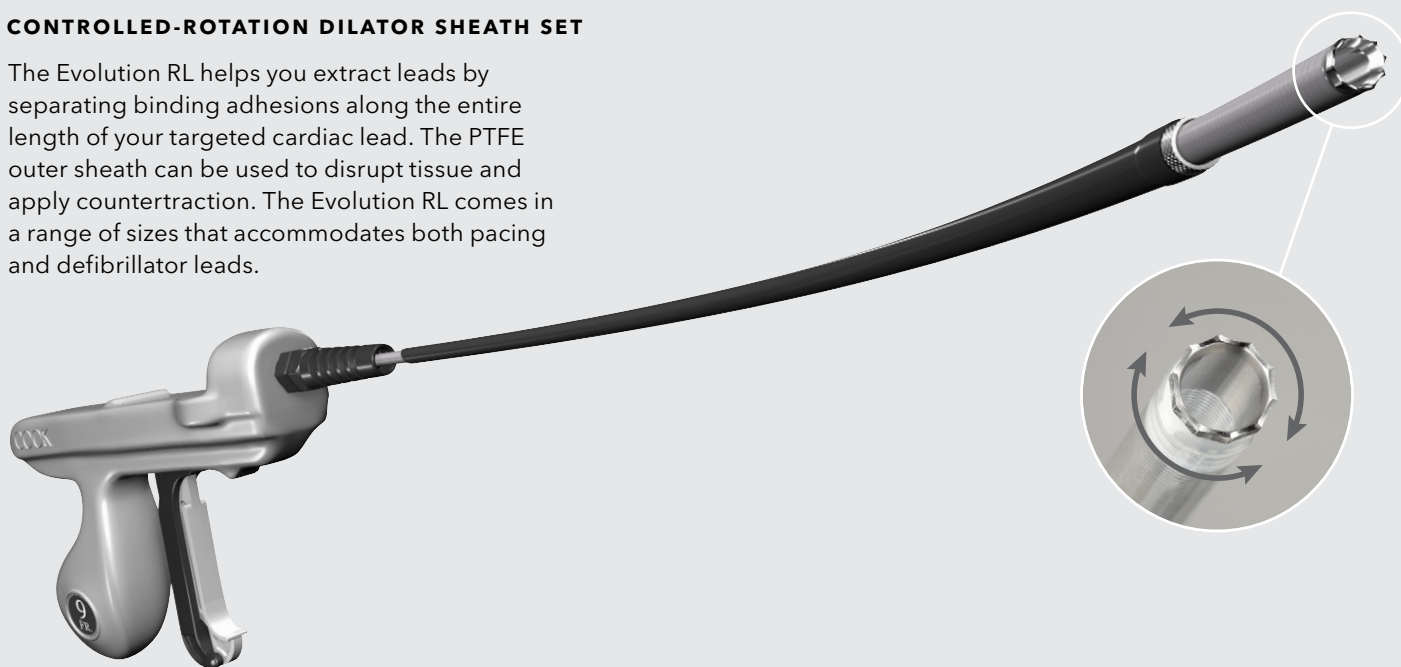

Evolution® Shortie RL

CONTROLLED-ROTATION DILATOR SHEATH SET

Designed specifically for vessel entry, the Evolution Shortie RL dilates scarred or calcified tissue bidirectionally around the targeted cardiac lead. The proprietary shape of the Evolution Shortie RL's decagonal tip allows the device to easily enter a vessel. The tabs on the outer sheath allow you to peel the sheath away more easily, so you can retain wire guides and, if necessary, reimplant the lead. The Evolution Shortie RL's shorter sheath gives you greater control.



Evolution® RL

LEAD EXTRACTION™ SYSTEM

Order Number	Reference Part Number	Inner Sheath ID Fr
Evolution RL		
G23737	LR-EVN-9.0-RL	9.0
G23746	LR-EVN-11.0-RL	11.0
G23747	LR-EVN-13.0-RL	13.0

Evolution RL is compatible with the following: Standard Outer Sheaths

		Compatible Sheath Fr
G26578	LR-PFTA-9.0-CS	9.0
G26586	LR-PFTA-11.0-CS	11.0
G26585	LR-PFTA-13.0-CS	13.0
SteadySheath Evolution Tissue Stabilization Sheath		
G25082	LR-TSS-9.0	9.0
G25083	LR-TSS-11.0	11.0
G25084	LR-TSS-13.0	13.0

Evolution Shortie RL

		Inner Sheath ID Fr
G23748	LR-EVN-SH-9.0-RL	9.0
G23749	LR-EVN-SH-11.0-RL	11.0

Evolution Shortie RL is compatible with the following: SteadySheath Evolution Shortie Tissue Stabilization Sheaths

		Compatible Sheath Fr
G31908	LR-TSS-SH-9.0	9.0
G 31923	LR-TSS-SH-11.0	11.0

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

Customer Service

EMEA: EDI - www.cookmedical.com/edi.do
Distributors: +353 61239240, ssc.distributors@cookmedical.com
Austria: +43 179567121, oe.orders@cookmedical.com
Belgium: +32 27001633, be.orders@cookmedical.com
Denmark: +45 38487607, da.orders@cookmedical.com
Finland: +358 972519996, fi.orders@cookmedical.com
France: +33 171230269, fr.orders@cookmedical.com
Germany: +49 6950072804, de.orders@cookmedical.com
Hungary: +36 17779199, hu.orders@cookmedical.com
Ireland: +353 61239252, ie.orders@cookmedical.com
Italy: +39 0269682853, it.orders@cookmedical.com
Netherlands: +31 202013367, nl.orders@cookmedical.com
Norway: +47 23162968, no.orders@cookmedical.com
Spain: +34 912702691, es.orders@cookmedical.com
Sweden: +46 858769468, se.orders@cookmedical.com
Switzerland - French: +41 448009609, fr.orders@cookmedical.com
Switzerland - Italian: +41 448009609, it.orders@cookmedical.com
Switzerland - German: +41 448009609, de.orders@cookmedical.com
United Kingdom: +44 2073654183, uk.orders@cookmedical.com

www.cookmedical.com

Americas: EDI - www.cookmedical.com/edi.do
Phone: +1 812.339.2235, 800.457.4500, Fax: 800.554.8335
E-mail: orders@cookmedical.com

Australia:
Phone: +61 738411188, 1800777222, Fax: +61 738411288, 1800077283
E-mail: cau.custserv@cookmedical.com

