



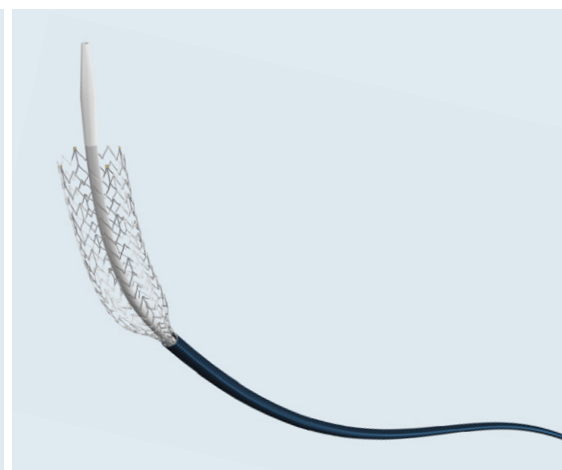

Zilver 635[®]

VASCULAR SELF-EXPANDING STENT

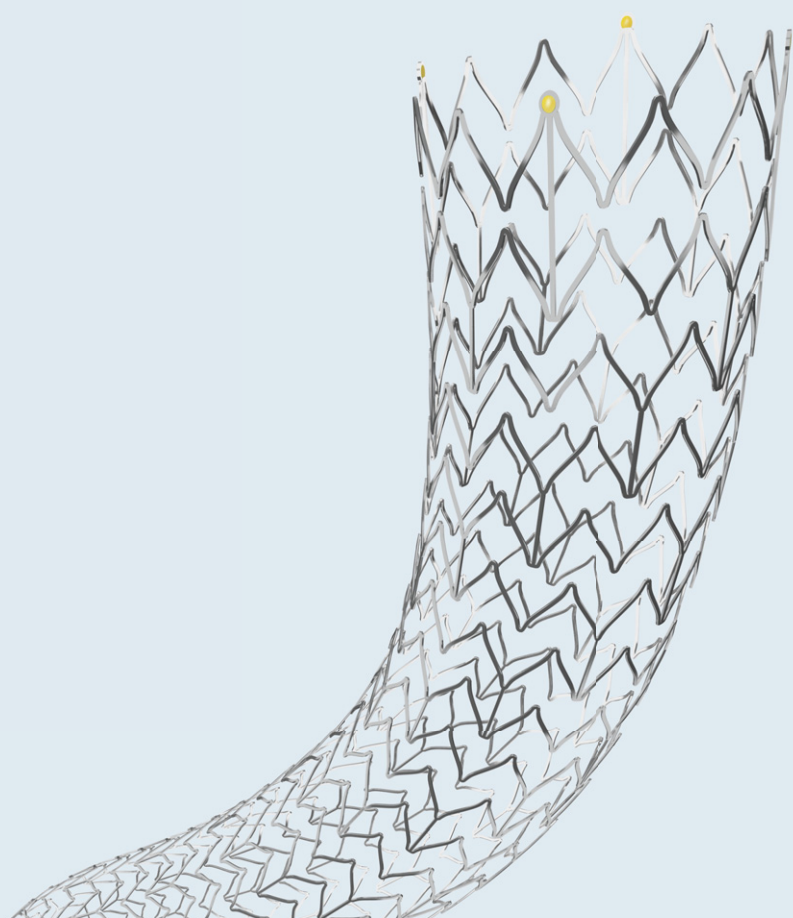

**Choose the iliac stent with
proven clinical performance.**

PROVEN DESIGN

The unique balance of flexibility, strength and durability means peak performance for your patient.

PROVEN PERFORMANCE

The Zilver[®] Vascular Stent has been clinically proven to maintain 92.9% patency in the iliacs at 9 months.¹

PROVEN DURABILITY

A recently-published retrospective review of iliac stenting revealed no fractures in the Zilver Vascular Stents.²



Zilver 635®

VASCULAR SELF-EXPANDING STENT

Global Product Number	Order Number	Stent Diameter mm	Stent Length mm
80 cm Delivery System			
G43844	ZIV6-35-80-6-20	6	20
G43845	ZIV6-35-80-6-30	6	30
G43846	ZIV6-35-80-6-40	6	40
G43847	ZIV6-35-80-6-60	6	60
G43848	ZIV6-35-80-6-80	6	80
G43849	ZIV6-35-80-7-20	7	20
G43850	ZIV6-35-80-7-30	7	30
G43851	ZIV6-35-80-7-40	7	40
G43852	ZIV6-35-80-7-60	7	60
G43853	ZIV6-35-80-7-80	7	80
G43854	ZIV6-35-80-8-20	8	20
G43855	ZIV6-35-80-8-30	8	30
G43856	ZIV6-35-80-8-40	8	40
G43857	ZIV6-35-80-8-60	8	60
G43858	ZIV6-35-80-8-80	8	80
G43859	ZIV6-35-80-9-20	9	20
G43860	ZIV6-35-80-9-30	9	30
G43861	ZIV6-35-80-9-40	9	40
G43862	ZIV6-35-80-9-60	9	60
G43863	ZIV6-35-80-9-80	9	80
G43864	ZIV6-35-80-10-20	10	20
G43865	ZIV6-35-80-10-30	10	30
G43866	ZIV6-35-80-10-40	10	40
G43867	ZIV6-35-80-10-60	10	60
G43868	ZIV6-35-80-10-80	10	80

Global Product Number	Order Number	Stent Diameter mm	Stent Length mm
125 cm Delivery System			
G43819	ZIV6-35-125-6-20	6	20
G43820	ZIV6-35-125-6-30	6	30
G43821	ZIV6-35-125-6-40	6	40
G43822	ZIV6-35-125-6-60	6	60
G43823	ZIV6-35-125-6-80	6	80
G43824	ZIV6-35-125-7-20	7	20
G43825	ZIV6-35-125-7-30	7	30
G43826	ZIV6-35-125-7-40	7	40
G43827	ZIV6-35-125-7-60	7	60
G43828	ZIV6-35-125-7-80	7	80
G43829	ZIV6-35-125-8-20	8	20
G43830	ZIV6-35-125-8-30	8	30
G43831	ZIV6-35-125-8-40	8	40
G43832	ZIV6-35-125-8-60	8	60
G43833	ZIV6-35-125-8-80	8	80
G43834	ZIV6-35-125-9-20	9	20
G43835	ZIV6-35-125-9-30	9	30
G43836	ZIV6-35-125-9-40	9	40
G43837	ZIV6-35-125-9-60	9	60
G43838	ZIV6-35-125-9-80	9	80
G43839	ZIV6-35-125-10-20	10	20
G43840	ZIV6-35-125-10-30	10	30
G43841	ZIV6-35-125-10-40	10	40
G43842	ZIV6-35-125-10-60	10	60
G43843	ZIV6-35-125-10-80	10	80

1. Krol KL, Saxon RR, Farhart N, et al. Clinical evaluation of the Zilver vascular stent for symptomatic iliac artery disease. *J Vasc Interv Radiol.* 2008;19(1):15-22.
2. Higashiura W, Kubota Y, Sakaguchi S, et al. Prevalence, factors, and clinical impact of self-expanding stent fractures following iliac artery stenting. *J Vasc Surg.* 2009;49(3):645-652.



www.cookmedical.com

COOK MEDICAL INCORPORATED
P.O. Box 4195, Bloomington, IN 47402-4195 U.S.A.
Phone: 812.339.2235, Toll Free: 800.457.4500, Toll Free Fax: 800.554.8335

COOK (CANADA) INC.
111 Sandiford Drive, Stouffville, Ontario, L4A 7X5 CANADA
Phone: 905.640.7110, Toll Free: 800.668.0300

WILLIAM A. COOK AUSTRALIA PTY. LTD.
95 Brandl Street, Brisbane Technology Park, Eight Mile Plains
Brisbane, QLD 4113 AUSTRALIA, Phone: +61 7 3841 1188

WILLIAM COOK EUROPE ApS
Sandet 6, DK-4632, Bjaeverskov, DENMARK, Phone: +45 56 86 86 86

© COOK 2009 PIL-2M-LTZ635DS-EN-200909